Medical Professional Testimonials



the first time. It shows significant scientific improvements of HIFU technology to develop great results. I believe Classys will be based on their outstanding technology."

"Ultraformer III's skin tightening effects are amazing. Laser technology has limitations in terms of clinical results and side effects. The

ing using HIFU that delivers energy, especially to the SMAS layer. The energy takes apart old collagen and induces formation of new collagen effectively."

....

which there is a high rate of patient satisfaction. HIFU devices have replaced the trend of RF devices recently because these devices like the

Ultraformer are more effective and is less painful. It helps with blood circulation and remodels collagen effectively."

Dr. Jong-seo Kim,

MD, Plastic Surgeon

Dr. Franco Lauro, MD, Plastic Surgeon



"Ultraformer III brings immediate tightening effects with different cartridges for the face. Surgery was the normal option for skin lifting procedures but now we can achieve equal results using the Ultraformer III non-

"For those who have never tried the Ultraformer III with HIFU technology, I'd like to say that this is a great tightening procedure device. We like to use it for tightening from the

eyes down to the neck. Patients reflect great results and they are highly satisfied."

ous. This is because we work on the tissues and various layers of the skin. With age, skincare products and cosmetics is just not enough. The Ultraformer is suitable for patients

Dr. Michael H. Gold,

MD, Dermatologist

Dr. Katia Paskova,

MD, Dermatologist





"I've been using the Ultraformer III for more than a year now and I am very satisfied with its clinical results. I believe the Ultraformer III is a game changer for skin lifting. Injections and surgery were options for skin lifting prior to



"The Ultraformer III is a very effective and sat-isfactory device that makes it possible to offer my patients a very complete treatment. I have before the Ultraformer III, I was not satisfied with other devices due to high pain levels and unsatisfactory clinical results."



for more than 6 months now. This is a very versatile device because there are cartridges ranging from 1.5mm up to 9.0mm. sagging skin on the face, but we are able to treat other areas of the body as well."



JF3B052017

ultraformer.com





T. +82-2-517-2114 | classys.com | ultraformer.com | info@classys.com

of both civil and criminal law of legal justice. Copyright to Classys © All Rights Reserved

The Classys Advantage

fat reduction, and body contouring procedures. Comfort coupled with beneficial, fast-proven results is the source of our motivation and the reason we strive to innovate solutions for our consumers in the medical & aesthetics industry.

Images and texts are intellectual property of Classys. Copying of this material can be subject to charges

MMFU I Micro & Macro Focused Ultrasound

Reform Your Youth



Lift Tighten Contour

The Ultraformer III is an optimum, non-invasive ultrasound device that lifts and tightens the face for a youthful complexion and tightens the body for slimmer contours. With precision per shot pulse, HIFU-powered transducers are designed to either remodel collagen to remove facial wrinkles and sagging skin or tighten body tissues to reflect your full potential.

Uplift your face, diminish those wrinkles, and shape your body



Multi-functional & Multi-depth Cartridges



Micro & Macro Focused Technology





Application Face & Body



Non-invasive Procedure Safety



Effective & Less Pain Treatment



Faster & Precise Shot Application Transducers




High Peak Power Dual Engine

Benefits for Patients

· Applicable for all skin types and tones

- · 15-20 minute treatments with NO downtime
- · No pre or post treatment skin care requirements
- · Quick and long-lasting results

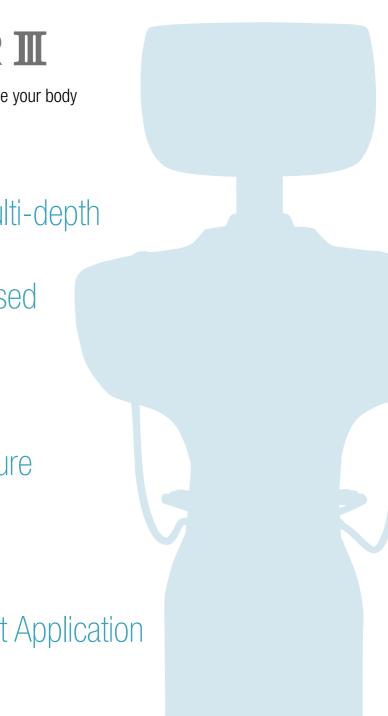

Benefits for Practice

- · Safe and effective alternative to Botox, invasive surgery
- · Customized treatment based on patient assessment
- · Complements other aesthetic treatments offered
- · Highly profitable and quick turnover on investment



Technology & Mechanism

HIFU transducers deliver an equal distribution of ultrasound waves into multiple layers of skin and body tissues without direct contact to the epidermis. Fitted with multiple cartridges that generate thermal energy, the Ultraformer III maintains stabilized temperatures of 65~75°C to induce coagulation for collagen renewal in the face and tightens body tissues for contouring waistlines, the thighs, and other parts of the body.

Neocollagenesis


Collagen renewal in the face triggered by HIFU involves heating the dermal and superficial muscular aponeurotic system (SMAS) layers that undergo separate phases of blood coagulation, wound contractions, and tighter shelving of new collagen to reduce wrinkles and sagging skin.


01 Inflammation Phase

Post treatment, the target area undergoes blood coagulation and hemostasis to control blood flow, which then induces a uniform migration of surrounding skin cells.

02 **Proliferative Phase**

48 hours after receiving treatment, fibroblasts produce new connective tissue known as granulation tissue to form on the wound, triggering a tighter build-up of new collagen.






Cell Migration

Wound Contraction

Micro Focused

Cartridges with highly concentrated ultrasound beams deliver power with accuracy and precision to the specified focal region.






Remodeling Phase

03


Over the course of 3 weeks to 6 months following treatment, the dermal layers of skin triggers renewal of cross-linked collagen fibers for a tighter and wrinkle-free complexion.




Skin Lifting & Tightening

Macro Focused

Cartridges with lower frequencies allow deeper penetration to the focal region with a larger energy density.

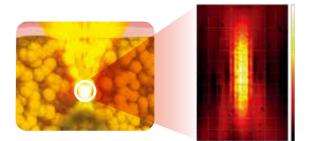

Technology

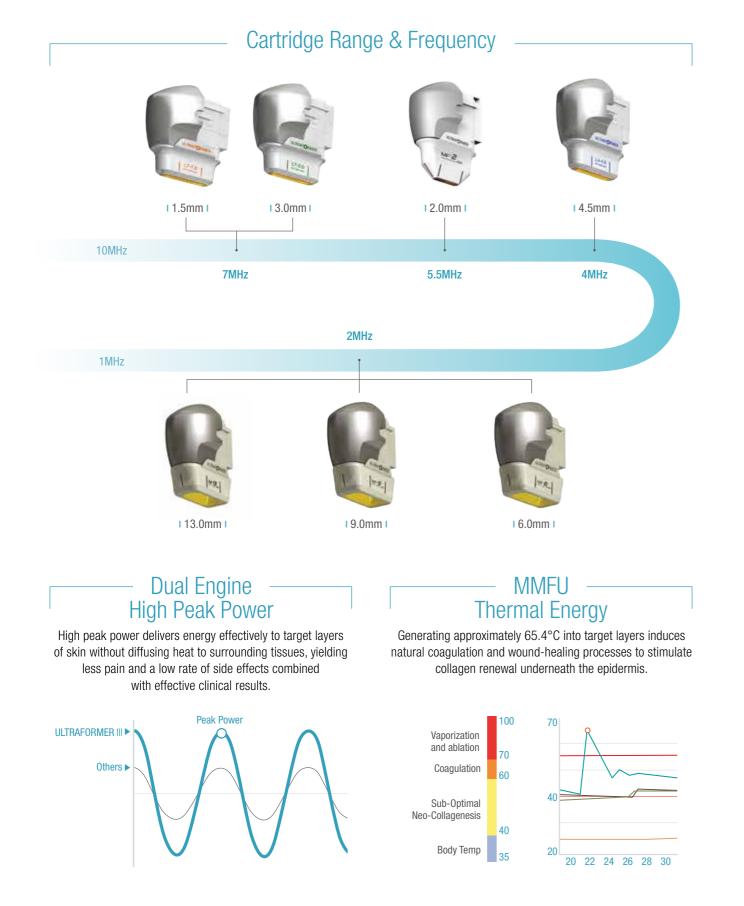

Brow Lifting Efficacy

Clinical Study Abstract

Over the course of 12 weeks, 30 patients participated in a clinical study to assess the efficacy of brow lift procedures using the Ultraformer III. Clinical photos were recorded at the start of each session to document improvement in results.







Baseline

Measurement of AEH Improvement

1.56^{mm}

90%

30

days

Patients evaluated in the course of 90 days achieved an average lifting effect of 1.56mm.

90% of 30 subjects receiving brow

lifts under clinical evaluation reported

significant lifting and tightening just

above the eyebrows 90 days post

30.5

30 29.5

29

The highest rate of clinical improvement was commonly recorded in the first 30 days following the first session of treatment.

28.5 28

Post Procedure

Post Procedure



Proven Efficacy Through Clinical Studies

Tightening effects of high-intensity focused ultrasound on body skin and subdermal tissue

[J Eur Acad Dermatol Venereol. 2016 Sep;30(9):1599-602.]

Research Abstract

Procedures with the Ultraformer III to increase skin elasticity in the face and tighten areas of the body through the non-invasive method of HIFU under multiple depth cartridges were evaluated to determine the efficacy of the device as a practical alternative to invasive procedures and surgery. The study was based on the standards of the Global Aesthetic Improvement Scale (GAIS) and elasticity changes to skin were measured via a cutometer.



The HIFU device used in this study was the Ultraformer III (CLASSYS INC.)

A Pain was evaluated by visual analogue scale (VAS) ... 1 and 4 weeks after treatment, all subjects reported a VAS score of 0 (no pain)

Most subjects were satisfied with the results of treatment (Table 2). At 4 weeks post-treatment, all subjects rated SGAIS scores as greater than 1 on the cheek and thigh. The improvement rate assessed for the abdomen as greater than SGAIS 1 was 93.8%. At 12 weeks post-treatment, the improvement rates of cheek and thigh were reduced from 100% to 96.9%. However, the improvement rate of the abdomen increased to 96.8%.)

Conclusion

For body tightening, we applied HIFU using transducers with a lower frequency and deep focal depth to effectively deliver ultrasound energy to skin tissues. HIFU appears to be a safe and effective treatment modality for dermal and subdermal tightening. W27 W28 W29 W30 W31 W32 W33 W34 W35

Proven Efficacy Through Clinical Studies Efficacy and safety of non-invasive body tightening with high-intensity focused ultrasound (HIFU)

[Skin Research and Technology 2017; 1-5]

Research Abstract

Clinical researchers have conducted treatment procedures on subjects with the Ultraformer III to determine whether high-intensity focused ultrasound (HIFU) is an effective, non-invasive alternative to incision-based procedures or surgeries for improving skin elasticity and contours of the face and body. Over the course of 12 weeks following treatment, researchers evaluated the device for its efficacy and safety based on the standards of the Global Aesthetic Improvement Scale (GAIS) and changes to skin elasticity measured over time via a cutometer.



LIGAIS scores also showe

66 Most subjects were satisfied with





Conclusion

In this study, we observed significant improvements in two body reg D North Amer for HIFU treatment. By using newly developed transducers with different energy outputs and focal depths, HIFU treatment can be tailored to meet the unique physical characteristics of each patient.

	_		WILEY
		WILEY	No. 2. Laskach HJ, Makin R, Barthe PG, Starton MH, Manthein D, Isterneto-
	dute-	all treated areas (Finure 2). The chance of the mean R7 value at the	⁶ cand drained evaluation of a two transmet modelly the perside minimage/attain within the data. Downstrating 2008;34(5):237-294. Kim Meilin, K., Kim M. Ubasanad akin tightening. Downaid Clin. 2014;42(1):75-77. Ki ¹² G. Caid St. Nu YK, Kim SI, Kim RJ, Kim MN, Tightening effects of high- regiment of the start o
WILEY	ributing	thish was 0.054s0.022, which represented the stratest change among	 Minis K, Alan M. Ultranand skin tighteeing. Dennatol Clin. 2014;22(1):75-77.
WILEY	t of the	the treated areas. IGAS scores also showed good results (Table 1). Of the three treated areas, the cheek demonstrated the greatest im-	IS. ⁴² S. Choi SY, Na YA, Kin SY, Kin BJ, Kin MN: Tighteeing effects of high- intensity focused ultrasaund on body skin and subdermal tissue: a
ody tightening with	utment,	provements after treatment. At 4 weeks post-treatment, the improve-	¹⁴¹ C. Markada (1977). ¹⁴² S. Markada (1977). ¹⁴³ S. Markada (1978). ¹⁴⁴ S. Markada (1978). ¹⁴⁵ Julie Carlo and J. Kanada (1978). ¹⁴⁵ Julie Carlo and J. K. Kanada (1978). ¹⁴⁶ All Carlo and Antonization (1978). ¹⁴⁷ S. Markada (1978). ¹⁴⁸ A. Markada (1978). ¹⁴⁸ S. Markada (1978). ¹⁴⁹ S. Markada (1978). ¹⁴⁰ S. Markada (1978). ¹⁴⁰ S. Markada (1978). ¹⁴⁰ S. Markada (1978). ¹⁴¹ S. Markada (1978). ¹⁴¹ S. Markada (1978). ¹⁴¹ S. Markada (1978). ¹⁴² S. Markada (1978). ¹⁴³ S. Markada (1978). ¹⁴³ S. Markada (1978). ¹⁴⁴ S. Markada (1978). ¹⁴⁴ S. Markada (1978). ¹⁴⁵ S. M
IFU)	test pa-	On our source stream data, are cleaned unconstant on graness are provements that relations. At 4 weeks pool vestings, the improve- ment rates of subjects who were assessed as either improved [GAMS cases 1] or much improved [GAMS cases 2] wave below, Below, and 78.1% on the cheek, abdomen, and thigh respectively. At 12 weeks	FIA: with transutaneous interest focused ultrasound. Dematti Surg. Deep 2012;20(5):55-759.
IFO)	d noon	78.5% on the cheek, abdomen, and thigh respectively. At 12 weeks	 with Transistaneou ubine focused ultrasout. Dematte larg. 2012.20(5):754-758. ack. Tolink N, EX X, Andred Gatley RA, Strangman NM, Kare M. A nor- danized, single-tilled, portmarketing study of multiple energy lewik.
	indomly intrusho		Kar- damibed, single-tiled, poctmarketing study of multiple energy levels of high-intensity focused diseasands for narionalise body subplice. Demonstati Say 2022;33(1):56-7. K of R. Shek SY, Young CK, Chan JK, Efficacy of high-intensity
¹ YJ. Jang ^{1,3} S. Y. Chol ^{1,4}	ectetic	to 90.6%, but the body areas did not change significantly. Most sub- jects were satisfied with the results of treatment (Table 2). At 4 weeks	x of B. Shek SY, Young CK, Chan JC, Chan HH. Efficacy of high-indensity Society ultrasanography for noninxasive lody sculpting in Chinese
	side-by-	post-treatment, all subjects rated SGAIS scores as greater than 1 on the cheek and thirds. The improvement rate assessed for the abdomen	view in starts in bang the chain of course of the start of a digitation of the start of the s
	ts using	are prater than SQAES two 92.08%. At 12 weeks pool-transmission of the advancement, the improvement rates of cheek and high were reduced from 500% to 94.9%. However, the improvement rate of the abdomen increased to	 Fanuk, Nije-istini, Kusari alkumani diselumina diselumi kana diselumi kan
	t 4 and Ouzaka	improvement rates of cheek and thigh were reduced from 100% to 96.9%. However, the improvement rate of the abdomen increased to	one pre-clinical and histological effects of subcataneous fat reduction wire hish-intensity focused ultranound in a sonise model. Skin Rec
htening devices have become increasingly popular for improvements in skin laxity and tightening with	city and	96.0%	Inclused 2017/22(2) 194-301. IFU 11. Nature M. Allan M. Perrodras E. et al. Skin Settemine induced by frac-
cy and safety of HIFU for skin tightening in the face	pecific R the total		Ting tonal CO, laws textment: quantified accessment of variations in me- salary chanical properties of the skin. J Costert Dematol. 2012;11:201-206.
icy and safety of HEFU for skin tightening in the face	tti were le (NRS)	TABLE 1 Investigator Global Aesthetic Improvement Scale (GAIS)	 Balan, 2012/22/19446. Hanna, 2012/22/19446. Hanna, Kan Manahan, Ku zi, Ki King Spinning Jankond Yu Yu- Yuang Xu, Yu X
bjects enrolled in this prospective clinical trial. The	2 weeks	IGAIS	unn spit fan tús with binded response euskados. Ach Dematol. ant 2006.142(8):965-990.
sects enrosed in this prospective cance their. The both cheeks, lower abdomen, and thigh. Skin elas- ter treatment using a Cutometer (CTS75, Courage "Dears Mindeal associational disensitieshite each		0 1 2 3	such 12. Ahn S, Kim S, Lee H, Muon S, Chang L Correlation between a Cutometer/R and quantitative evaluation using Mole topography in
ter treatment using a Cutometer (CT575, Courage Three blinded exercises of demotionists evalu-		Cheek	Cutameterft and quartitative exclusion is using Main tapography in age-widead disi existing Sinis Bachust 2003;132(200-364, 54, Stanger N, Landberg G, Chines M, Karlen M, Kernisten M, Age- midded changers in disi metrical properties: a quantitative evalua- tion of 120 break-anajors. Sinis Ref. Endows 2015;175(216-361, Stangers 2015). Sinis Ref. Sinis Ref. Stangers 2015;175(216-361, Stangers 2015). Sinis Ref. Stangers 2015;175(216-361, Stangers 2015;175
Three blinded, experienced dermatologists evalu- nt (week 4 and 12) photographs according to the icale (GAIS). Participants also completed self-		Pud-toutnent n 1 29 2 0 (4W) % 31 954 43 0	related changes in skin mechanical properties: a quantitative evalua- tion of 120 female subjects. Skin Rec Technol. 2011;17(2):141-548.
	015-12-	(WM) % 3.1 90.6 6.2 0 Puct-seatness n 3 2.9 0 0 (%2W) % 9.4 90.6 0 0	
ated their pain on a numeric rating scale (NRS) im- weeks after treatment.	multiple	(12W) % 9.4 90.4 0 0	How to cite this article: Ko E1, Hong JY, Keon T-R, et al.
case (LACA), i-varticipants and completion sen- ated their pain on a numeric rating scale (NRS) im- weeks after treatment. Is a Cutometer was significantly improved 12 weeks (Pv.05), Both ISARS and SSARS showed significant isom homodified in the numeric the more NRT	tandard	Past-teatment n S 27 0 0	How to close this articles (Is. E1, Hong JP, Kucol T-R, et al. Efficacy and suffery of non-invasion body fightening with high-high-hierandry focused transmost (FHC), Bio Re Tarbacol. 2017;00:1-5. https://doi.org/10.1111/wt12271
P<.05]. Both IGAIS and SGAIS showed significant	0Z.	(4W) % 15.6 84.4 0 0	regn-intensity tocased ultrasound (HFU). Skin Rei Technol. 2017;00:1-5: https://doi.org/10.1111/urt12271
was reported at 4 and 12 weeks post-treatment		Past-teatment n 5 26 1 0 (12W) % 15.6 81.2 2.1 0	
meet. Immediately after treatment the mean NRS was reported at 4 and 12 weeks post-treatment. served during the follow-up period.		Thigh	
ively improves skin elasticity and clinical contour-		Put-tnutnent n 7 25 0 0 (4W) % 21.9 78.1 0 0	
	n), aged and IV.	Put-treatment n 7 25 0 0	
		(12W) % 21.9 78.1 0 0	
	dicatily wlice in	0-No charge, 1-Mid improvement, 2-Moderate improvement, 2-Significant improvement.	
Radiofrequency and infrared laser devices which expose			
ar senseed test and stimute neccolagenesis in de- lefor efficacy so that surgery still remains the treatment			
moderate to severe tissue lasity. ¹ Although surgical face			
Redefinguency and infranced tames devices which response to controlled the anal of chandre monoclusprenesis in der- flerfor efficacy on that surgery call measures the transment in noderatio to unwave time kingle All-back processing the interact the transmerse to improve data backs, it is also in not effective transmerse to improve data backs, it is also that handware data surveit as infrances, more dam- et risks of anotherials, useding, and handing 24 enclosurgers an onlygingle used as a non-invasione modeling why destroying tamor cells of internal organs by thermal		Address of the second	
nt risks of assetthecia, novelling, and braising ² echnology was printedly used as a non-invasion module.		The second second second	
ely destroying tamor cells of internal organs by thermal	Chevrile.	Abdumen Tingh P <coolservus. by<br="" lefture="">pained samples inted Culture (RT) Incl.</coolservus.>	
c C 2017 John Wiley & Sons A/S. 1 Buildead to: Max Wiley & Sons 1/d			
Published by John Wiley & Sons 21d			
good results	(Ta	ble 1). 77	
		ble 1). 77 tment (Table 2) ,	
			08 09 20
			60 80
		It ment (Table 2)	WILEY 1 3 will be a start IT value at the movement of the practice Unique among a draw changed group issuits; (black t) cheak demonstrated the groupster ar-
good results ne results of t		tment (Table 2)	WILEY 4 will be a set of the set
		All treated oness (Flager 2)	WILEY - 3 c charge of the smark R7 value at the many tort of the pratect During among an aba to change good markity (dath H) e check domonitated the pratect ar- t4 works pool thramptone. The improve reasonable at alther inproved GMB
e results of t		All treated oreas (Flowr 2) all treated oreas (Flowr 2) The tright ways 0.054+p0.002; which the treated areas, the order the treatment areas, the processments after treatment. A most rates of subjects who as sone 3) or much improved (2)	WILEY 3 a charge of the water R7 value at the mainted the gradient charge among in abus channel good instant, Glade E1 cheast damaschardt the gradient ar- ted waters an ather insported (GMB skills ruper 2) areas (55%, 5448), and
e results of t		All treated oreas (Flowr 2) all treated oreas (Flowr 2) The tright ways 0.054+p0.002; which the treated areas, the order the treatment areas, the processments after treatment. A most rates of subjects who as sone 3) or much improved (2)	WILEY - 3 c charge of the smark R7 value at the many tort of the pratect During among an aba to change good markity (dath H) e check domonitated the pratect ar- t4 works pool thramptone. The improve reasonable at alther inproved GMB
e results of t		All transformers (Table 2)	WILEY 4 to charge of the main RV value at the mounter of the particle charge among a charge of the main RV value at the mounter of the particle charge among a charge domain that is particle ar- t is working of the mounter that improve we assume at an other incomed (03A6 345) score 2) answ 95.9%, 54.4%, and and trage separcherly AL2 severs
		All traded onesi (Figure 3) Th degraws 0.05450 002, which the base to 0.05460 002, which the traded area. We off the three traded areas, the provement affect traded areas.	WILEY ¹³ c charge of the what R7 value at the many nord the pratect charge around an advancement of the pratect ac- t water channel dependence. the improve a source of a within the pratect ac- t water prove the strength of GMB (AdS strength as the theorem of GMB as and triagn respectively. At 12 weeks on tange of the choice and wate reduced
e results of t		All traded onesi (Figure 3) Th degraws 0.05450 002, which the base to 0.05460 002, which the traded area. We off the three traded areas, the provement affect traded areas.	WILEY 4 to charge of the main RV value at the mounter of the particle charge among a charge of the main RV value at the mounter of the particle charge among a charge domain that is particle ar- t is working of the mounter that improve we assume at an other incomed (03A6 345) score 2) answ 95.9%, 54.4%, and and trage separcherly AL2 severs
e results of t		the traded oreas (fleer 2), at traded oreas (fleer 2), the traded area, 10,000 of the first traded area, 10,000 of the first traded area, 10,000 or one take of autoch who are not take of autoch who are not take of autoch who areas the traded areas, address to 40,515 to the observed (0).	WILEY ¹³ c charge of the what R7 vides at the many nord the pratect budge around an abuse channel produced to the pratect ar- t waters to develop the statement. The improve expansion an attement the improve or auxiliary and within the pratect ar- t waters to develop the statement. The improve expansion at within the pratect all of the statement and the improve of statement and the improve of statement and the improve expansion and the improve of statement and the improve expansion
e results of t		All treated oness (Figure 2) and treated oness (Figure 2) and treated ones. (Figure 2) and (Figure	WILEY
e results of t		the entry of the second	WILEY 3 a charge of the smart R7 where it the is charge of the smart R7 where it the to explore the smart R7 where it the to explore the smart R7 where it the is well they is expectively. At 12 weeks on the charge respectively. At 12 weeks of the charge respectively. At 12 weeks
e results of t		All transford onesis (Filtery & The right was 0.0541±0.002, which the Theoder Areas, Table Care Of the Hove transford Area (Table Care Of the Hove transford Area), and the proceeding of additional areas, the proceeding of additional areas, and the proceeding of a statement of the Additional areas, and the proceeding of a statement of the Additional and the pro- port freedoment of additional and the observed on the Mark Table Incore the Ob	WILEY
e results of t		All transford onesis (Filtery & The right was 0.0541±0.002, which the Theoder Areas, Table Care Of the Hove transford Area (Table Care Of the Hove transford Area), and the proceeding of additional areas, the proceeding of additional areas, and the proceeding of a statement of the Additional areas, and the proceeding of a statement of the Additional and the pro- port freedoment of additional and the observed on the Mark Table Incore the Ob	WILEY
e results of t		All treated oreas (Flager 2) all treated oreas (Flager 2) the second oreas (Flager 2) the second or 2) the second or 2) (All the stree treated oreas, the provement able treatment, All all case (All the stree treatment, and was to the offens, able the post freetment, the instruction to 90.6%, but the instruction to 90.6%, but the instruction to 90.6% but the instruction and the scattering of the ore post freetment, the instruction and the scattering of the ore post freetment, the instruction and the scattering of the ore or the ore one the ore of the ore or the ore one ore one	WILLEY
e results of t		the entry of the set o	WILEY - 3 to charge of the smark RT value at the mounted of the gradient and a to charge of the smark RT value at the mounted of the gradient and a data beamed good means. Claich RI to value a down of the state of the probability of the state of th
e results of t		the entry of the set o	WILLEY
e results of t		All treated onesis (Fileer 2), all treated onesis (Fileer 2), the fileer 2002, which the fileer area. (Fileer 2002, which the fileer area.) (Fileer 2002, File processes and subjects where are set of subjects where area.) performer and fileer 2002, file and fileer area.) (Fileer 2002, file area areas and file and file file area filearisment, solid area.) area filearisment, solid area.) area filearisment, solid area (Filear 4) \$3.75. Intervent, the improvement	WILEY - 2 to charge of the mean RT value at the movement of the products of the movement of the products of the product of the relevant downed good means, Claich II is check downeod the product of the product of the product of the product of the works and there increased (CMB 45% values 2) wave 65% R-144.8%, and is with the increased the product of the the state of the checks and products of the state of the checks and products of the St-0.5% comes an guester that is a revenue rate accessed for the abdoment 13% R-12 waves pool treatment, the met thigh were modered them TODs in met case of the dodoment new Store in the state of the state of t
e results of t		the entry of the set o	WILEY - 3 c charge of the smark RT value at the mounted of the grant RT value at the mounted of the grant states are at the charge of the state in the states at the charge of the states in the states of the value of the states in the states of the states of the states in the states of the states of the states in the states of the states of the states of of the states of the states of
e results of t		All treated onesis (Fileer 2), all treated onesis (Fileer 2), the fileer 2002, which the fileer area. (Fileer 2002, which the fileer area.) (Fileer 2002, File processes and subjects where are set of subjects where area.) performer and fileer 2002, file and fileer area.) (Fileer 2002, file area areas and file and file file area filearisment, solid area.) area filearisment, solid area.) area filearisment, solid area (Filear 4) \$3.75. Intervent, the improvement	WILEY - 2 to charge of the mean RT value at the movement of the products of the movement of the products of the product of the relevant downed good means, Claich II is check downeod the product of the product of the product of the product of the works and there increased (CMB 45% values 2) wave 65% R-144.8%, and is with the increased the product of the the state of the checks and products of the state of the checks and products of the St-0.5% comes an guester that is a revenue rate accessed for the abdoment 13% R-12 waves pool treatment, the met thigh were modered them TODs in met case of the dodoment new Store in the state of the state of t
e results of t		All treated onesis (Fileer 2), all treated onesis (Fileer 2), the fileer 2002, which the fileer area. (Fileer 2002, which the fileer area.) (Fileer 2002, File processes and subjects where are set of subjects where area.) performer and fileer 2002, file and fileer area.) (Fileer 2002, file area areas and file and file file area filearisment, solid area.) area filearisment, solid area.) area filearisment, solid area (Filear 4) \$3.75. Intervent, the improvement	WILEY - 2 to charge of the mean RT value at the movement of the products of the movement of the products of the product of the relevant downed good means, Claich II is check downeod the product of the product of the product of the product of the works and there increased (CMB 45% values 2) wave 65% R-144.8%, and is with the increased the product of the the state of the checks and products of the state of the checks and products of the St-0.5% comes an guester that is a revenue rate accessed for the abdoment 13% R-12 waves pool treatment, the met thigh were modered them TODs in met case of the dodoment new Store in the state of the state of t
e results of t		All treated onesis (Fileer 2), all treated onesis (Fileer 2), the fileer 2002, which the fileer area. (Fileer 2002, which the fileer area.) (Fileer 2002, File processes and subjects where are set of subjects where area.) performer and fileer 2002, file and fileer area.) (Fileer 2002, file area areas and file and file file area filearisment, solid area.) area filearisment, solid area.) area filearisment, solid area (Filear 4) \$3.75. Intervent, the improvement	WILEY - 2 to charge of the mean RT value at the mounted of the gradient and the mounted of the gradient and the related download the gradient and to whole you brademont. Builingtone as and these interview of SNR, 64448, and as and they inspectively. At 12 weeks and and the theorem of SNR, 64448, and and the formation and provide the and and the formation and provide the and and the formation and provide the and the SL-AN comes positionation, the and and SL-AN comes positionations.
e results of t		All treated onesis (Fileer 2), all treated onesis (Fileer 2), the fileer 2002, which the fileer area. (Fileer 2002, which the fileer area.) (Fileer 2002, File processes and subjects where are set of subjects where area.) performer and fileer 2002, file and fileer area.) (Fileer 2002, file area areas and file and file file area filearisment, role of file af 93.75. Intervent, the instrumer	WILEY - 3 c charge of the smark RT value at the mounted of the grant RT value at the mounted of the grant states are at the charge of the state in the states at the charge of the states in the states of the value of the states in the states of the states of the states in the states of the states of the states in the states of the states of the states of of the states of the states of
e results of t	rea	the end of	WILEY - 3 c charge of the smark RT value at the mounted of the grant RT value at the mounted of the grant states are at the charge of the state in the states at the charge of the states in the states of the value of the states in the states of the states of the states in the states of the states of the states in the states of the states of the states of of the states of the states of

SEURODE

Applications


Face

Micro focused depth cartridges at 1.5mm, 2.0mm, 3.0mm, and 4.5mm directly transfer an equal distribution of ultrasound energy into the dermal and superficial muscular aponeurotic system (SMAS) layers of the face to stimulate collagen renewal.



Body

Macro focused depth cartridges at 6.0mm, 9.0mm, and 13.0mm directly transfer an equal distribution of ultrasound energy into the subcutaneous tissue, inducing contractions to dispose of stubborn fat cells naturally through the body as waste.

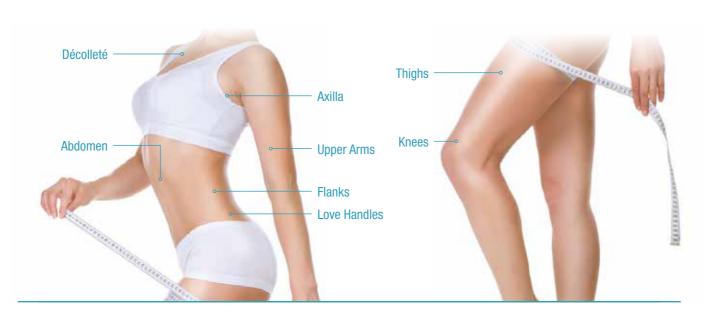

FAQ

What are the advantages of the Ultraformer III?

The Ultraformer III utilizes cartridges focused on multiple depths of skin for lifting and tightening the face as well as tightening body tissues for contouring purposes. The patient can receive customized treatments on the face and body with the stable delivery of ultrasound energy, fast application, and precise accuracy of MMFU-powered transducers.

How is fat naturally removed from the body by the Ultraformer III?

Macro-focused depth cartridges damage fat cell membranes consisting of triglycerides and are then transported through the vascular and lymphatic systems to the liver. This process is made possible through the body's natural metabolism as the liver makes no distinction between fat disposed of by the Ultraformer III and fat originating from food consumption.

Are there any side effects?

Although competitive results for facial lifting and tightening and body contouring will likely show over the next 3 months post treatment, patients may still experience slight redness for a few hours as well as swelling or tingling in either treatment area for up to a few weeks. There may also be bruising and numbness on treated areas but should resolve 2-4 weeks following procedure.

Is there any pain during treatment?

The Ultraformer III delivers comfortable procedures with its uniquely-designed transducer system developed only by CLASSYS. Many patients and practitioners report that the Ultraformer III, in comparison with other devices, delivers minimal pain with slight discomfort to the face or body, though sensations quickly subside immediately following treatment.

Am I a candidate for the ULTRAFORMER III?

Patients with diverse skin conditions such as fine lines, wrinkles, and hyperpigmentation on the face, or stubborn belly fat and love handles desiring a more curvaceous body figure, serve as ideal candidates for the Ultraformer III. Practitioners can also accommodate both face and body profiles with a variety of multi-depth cartridges that cater to a larger demographic of candidates.



Face I Lifting & Tightening

Participants shown in the following clinical photos received one ULTRAFORMER III treatment on the target areas presented. Evidence of clinical photos obtained from baseline and post procedure measurements indicates results in progress.

I noticed a much brighter complexion after receiving my first Ultraformer III treatment. I'm now confident to say goodbye to those fine lines and wrinkles. 99

- Sarah Newman, 50 -


I was amazed at how the Ultraformer III could treat the narrow contours of my face. Not only that, I can go straight to work right after treatment!

- Nicole Sutherland, 36 -







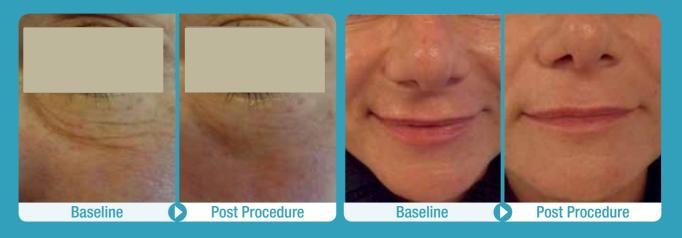

× Individual results may vary. Unretouched photographs.

Body I Tightening & Contouring

Participants shown in the following clinical photos received one ULTRAFORMER III treatment on the target areas presented. Evidence of clinical photos obtained from baseline and post procedure measurements indicates results in progress.




× Individual results may vary. Unretouched photographs.

The Classys Advantage

Providing Tools for Your Success

When partnering with a company with a global technology standard, a matching standard of support is a necessary tool to help with maximizing your success. Active on all mainstream networks in our day and age, Classys provides a top tier support service that caters to your practice.

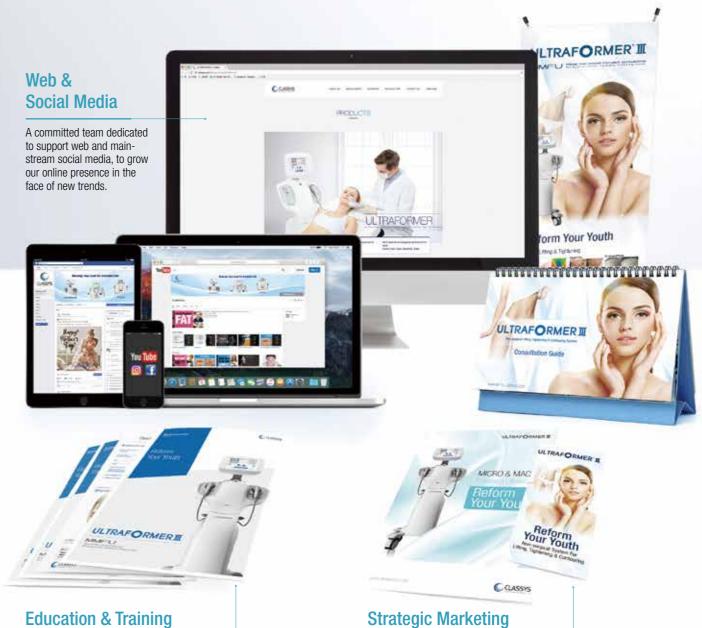

Providing practitioners with a comprehensive package of tools, knowledge, and training for the proper and professional use of our technologies.

A live database of dynamic content and material, suitable for both B2B and B2C end-users operating in globally diverse markets.